UNIUM™ System

Care and Maintenance

DePuy Synthes
THE ORTHOPAEDICS COMPANY OF Johnson & Johnson

Disassembly

Modular Handpiece Attachments



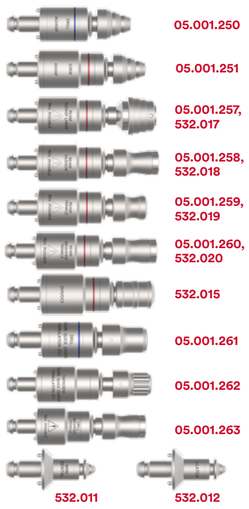

Reciprocating Saw Handpiece Accessory

** available in USA only

1a Manual Cleaning

Manual Cleaning



Disinfection







1b Automated Cleaning

Manual Pre-Cleaning



Cleaning and Disinfection

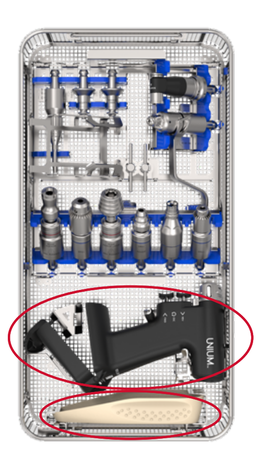







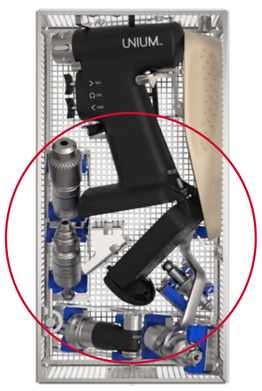



2 Lubricating

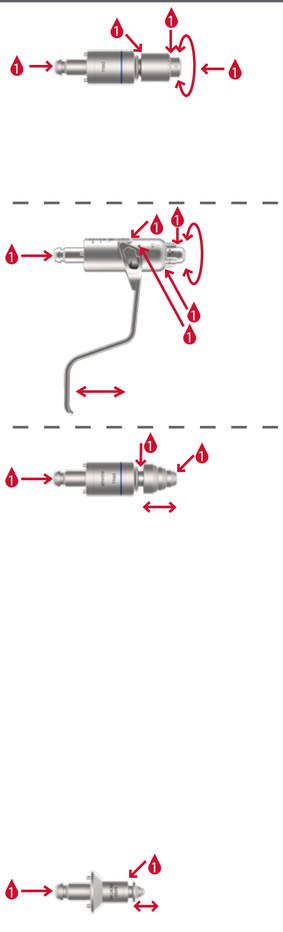

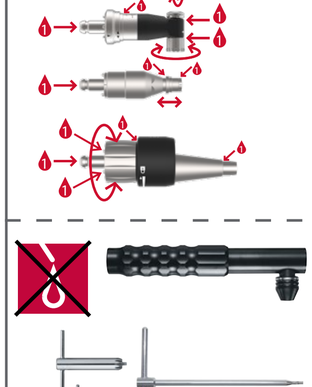

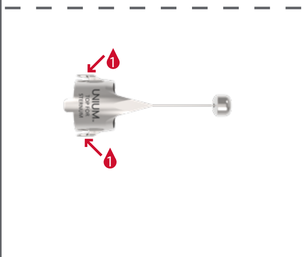

3 Check Function

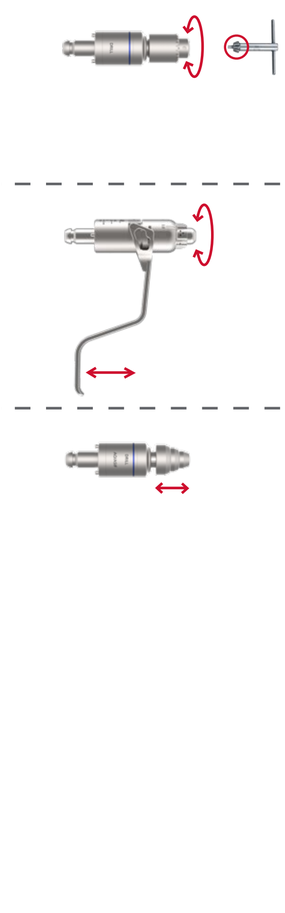

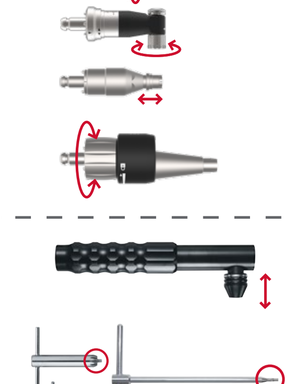

4 Sterilization

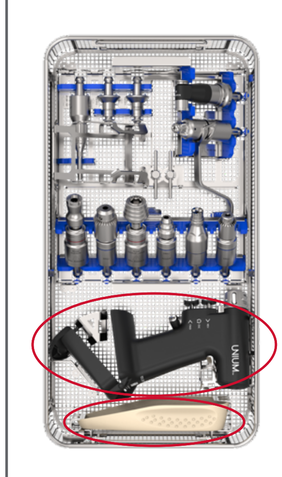



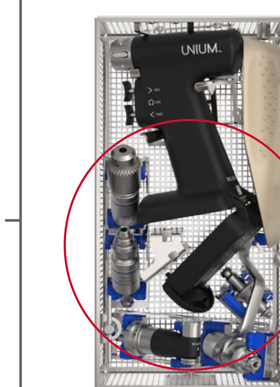



PICTOGRAM KEY

Explanation of the pictograms used in the poster

Note: Symbols shown at the top of each Care and Maintenance step in the poster apply to all article groups, if not indicated differently.



When a symbol in the poster is marked with a cross, the action is forbidden. Not following this may result in damage to the product and patient or user harm.

Caution: Use the mentioned article for this step

Disassembling

Spray with disinfectant and wipe off*

Immersion in disinfectant possible*

Wipe off with an absorbent cloth soaked in disinfectant*

Manual cleaning

Automated cleaning with manual pre-cleaning

Immersing allowed

Immersing and automated cleaning allowed

Check the function of parts marked in red

Lubricate the designated points. See product-specific “Instructions for Use” for more detailed information

Steam sterilization

Hot air, ethylene oxide, plasma and formaldehyde sterilization

H_2O_2 plasma STERRAD sterilization (max. 60 °C/140 °F)

H_2O_2 V-PRO sterilization (max. 50 °C/122 °F)

Do sterilize!

Please refer to the instructions for use of UNIUM and Universal Battery Charger II for a complete list of indications, contraindications, warnings and precautions.

All Synthes implant instructions for use as well as other instructions for use are available as PDF files at www.e-ifu.com.

Not all products are currently available in all markets.

Please contact your DePuy Synthes sales representative for more information.

CAUTION: United States Federal law restricts these devices to sale by or on the order of a physician

* Follow disinfectant manufacturer’s instruction.

** Refer to product label for legal manufacturer.

www.jnjmedtech.com

Synthes GmbH
Eimattstrasse 3
4436 Oberdorf
Switzerland
Tel: +41 61 965 61 11

Synthes GmbH
Luzernerstrasse 21
4528 Zuchwil
Switzerland
Tel: +41 32 720 40 60

© DePuy Synthes 2023. All rights reserved.
165764-230821 DSUS/EMEA
Issued 08/2023