

## Implant Bespoke Report for:

DePuy

## Corail Stem (Collared Stem with Pinnacle Cup)

Comprising PRIMARY hips implanted up to:	07 March 2021
NJR Database extract:	06 May 2021
Produced on:	15 June 2021
Licensed for use until:	15 June 2023

## Contents

Recorded Usage in NJR	2
Patient and Procedure Details	3
Revision and Survivorship	4
Patient Reported Outcome Measures	12
APPENDIX A – Component List	17

This report has been produced by the National Joint Registry of England, Wales and Northern Ireland (NJR). It summarises usage and outcomes associated with the Corail Stem (Collared Stem with Pinnacle Cup) up to the specified dates. This analysis is based on data collected by the NJR and PROMs data collected by NHS Digital for the following combinations of products:

<b>Femoral components</b>	<b>Corail Stem (Collared Stem with Pinnacle Cup)</b>
<b>Acetabular Component</b>	<b>Pinnacle cups (excluding metal liners)</b>
<b>Comparator Group</b>	<b>All NJR Hybrid Hips (excluding MoM)</b>

Appendix A lists details of all Corail Stem components included in this report.

This report is subject to the National Joint Registry Supplier Feedback Terms and Conditions Use. In particular,

**NJR Recorded Usage**

**Implant Usage**



Date of first recorded usage in the NJR: **11 January 2004**

Date of last recorded usage in this dataset: **07 March 2021**

Maximum implantation time: **17.2 years**

Mean implantation time: **4.8 years**

Totals Recorded in NJR	Cumulative Total
Procedures	102,823
Patients	92,576
Centres	340
Consultants	1,219
Implanting Surgeons	2,061

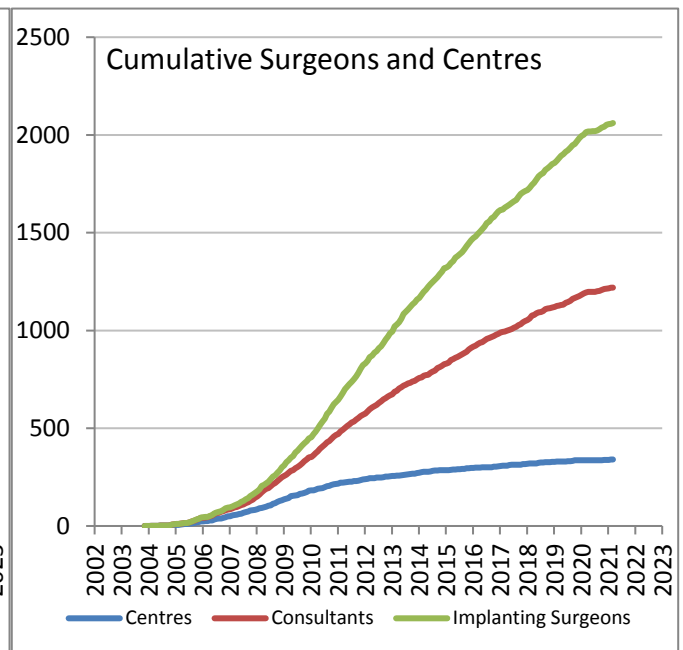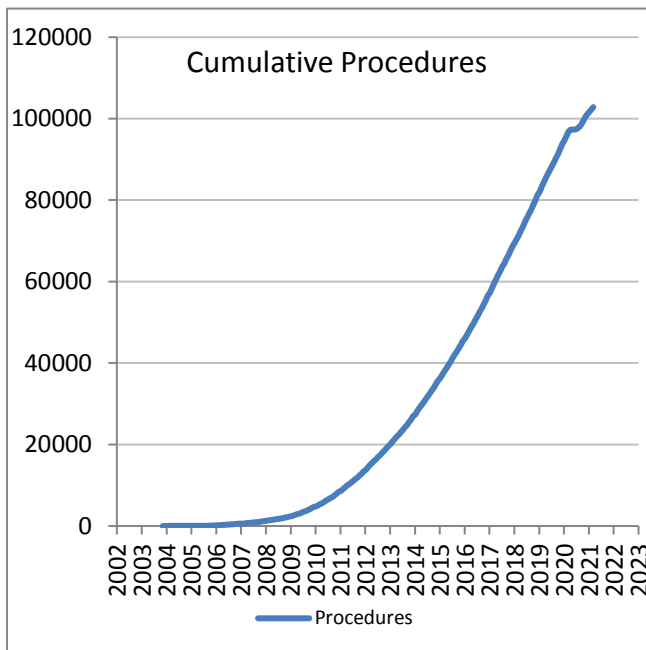

Current Outcome	Year of implantation													Total	%
	Pre-2010	2010	2011	2012	2013	2014	2015	2016	2017	2018	2019	2020	2021		
<b>Death</b>	1295	853	1020	1028	1066	955	777	714	505	332	186	32	0	8763	8.5%
<b>Revised</b>	167	103	126	146	129	130	156	152	130	108	67	27	3	1444	1.4%
<b>Unrevised</b>	3341	2811	3940	5186	6101	7745	8869	10347	11503	12118	12305	7069	1281	92616	90.1%
<b>Total</b>	<b>4803</b>	<b>3767</b>	<b>5086</b>	<b>6360</b>	<b>7296</b>	<b>8830</b>	<b>9802</b>	<b>11213</b>	<b>12138</b>	<b>12558</b>	<b>12558</b>	<b>7128</b>	<b>1284</b>	<b>102823</b>	<b>100%</b>

## Patient / Procedure Details

## Patient Details

	Corail Stem (Collared Stem with Pinnacle Cup)	All other Hybrid Stems Exl MoM	All NJR hip replacement
<b>Total Procedures</b>	102,823	298,465	1,285,207
<b>Total Patients</b>	92,576	266,742	1,082,079
<b>Demographics</b>			
Mean age	<b>66.5</b>	<b>69.7</b>	<b>68.6</b>
< 50	6.7%	4.6%	5.9%
50 – 59	17.9%	11.7%	13.8%
60 – 69	33.8%	28.3%	28.9%
70 – 79	30.7%	37.5%	34.7%
≥ 80	10.9%	18.0%	16.6%
Median BMI	<b>28</b>	<b>28</b>	<b>28</b>
% BMI information available	74.3%	69.2%	62.7%
Underweight ( BMI < 18.5)	0.7%	1.0%	0.9%
Normal (18.5 ≤ BMI < 25)	18.7%	21.7%	20.8%
Overweight (25 ≤ BMI < 30)	38.9%	39.1%	39.6%
Obese I (30 ≤ BMI < 35)	27.1%	25.2%	25.8%
Obese II (35 ≤ BMI < 40)	11.1%	9.6%	9.7%
Obese III (BMI ≥ 40)	3.6%	3.3%	3.3%
% Male	42.3%	37.4%	40.2%
<b>ASA Grades</b>			
P1 - Fit and healthy	15.0%	12.9%	15.6%
P2 - Mild disease not incapacitating	71.5%	68.4%	67.7%
P3 - Incapacitating systemic disease	13.2%	18.1%	16.2%
P4 / P5	0.4%	0.6%	0.6%
<b>Indications</b>			
Osteoarthritis	94.20%	88.74%	91.26%
Rheumatoid Arthritis	0.95%	1.53%	1.32%
Avascular Necrosis	1.95%	2.92%	2.53%
Fractured Neck of Femur	2.40%	5.77%	3.69%
CDH/DDH	1.31%	1.81%	1.58%
Other	0.96%	2.24%	2.12%

Total of indications may exceed total number of implants, since more than one indication can be listed per case.

**Revision and Survivorship**

**Reasons for Revision - excluding Metal on Metal**

Reasons for revision of non-MoM primary procedures in which the implant was used.

Reason for Revision	Revised <sup>†</sup>	Expected Revisions <sup>*</sup>	p value
Unexplained Pain	106	113.59	0.479
Dislocation / Subluxation	328	389.80	<0.001
Adverse Soft Tissue Reaction	35	44.50	0.146
Infection	279	374.56	<0.001
Aseptic Loosening - Stem	333	242.99	<0.001
Aseptic Loosening - Socket	71	90.75	0.025
Periprosthetic Fracture Stem	107	311.15	<0.001
Periprosthetic Fracture Socket	13	34.65	<0.001
Malalignment Stem	63	52.54	0.11
Malalignment Socket	102	93.38	0.337
Wear Of Acetabular Component	51	51.30	1
Lysis Stem	25	29.75	0.439
Lysis Socket	13	19.12	0.185
Implant Fracture Stem	13	24.49	0.012
Implant Fracture Socket	54	35.98	0.002
Implant Fracture Head	4	8.14	0.129
Dissociation of Liner	54	42.75	0.065
Other / Not recorded	68	71.20	0.745
<b>Total Revised</b>	<b>1444</b>	<b>1706.53</b>	<b>&lt;0.001</b>

\* Based on All Hybrid Stems Exl MoM (excluding metal on metal), adjusted for agegroup, gender, indications, and implantation year

† multiple reasons may be listed for one revision procedure

- Significantly better, p < 0.001
- Significantly better, p < 0.05
- Significantly worse p < 0.05
- Significantly worse p < 0.001




Components Revised	Number of procedures	Corail Stem (Collared Stem with Pinnacle Cup)	All other Hybrid Stems Exl MoM
Femoral only	419	29%	30%
Acetabular only	354	25%	19%
Both femoral and acetabular	406	28%	37%
Neither femoral nor acetabular revision recorded *	265	18%	14%

\* includes isolated head and/or liner exchange

Revision and Survivorship

Cumulative Revision Rate

Endpoint: All reasons for revision. Excluding Metal-on-Metal

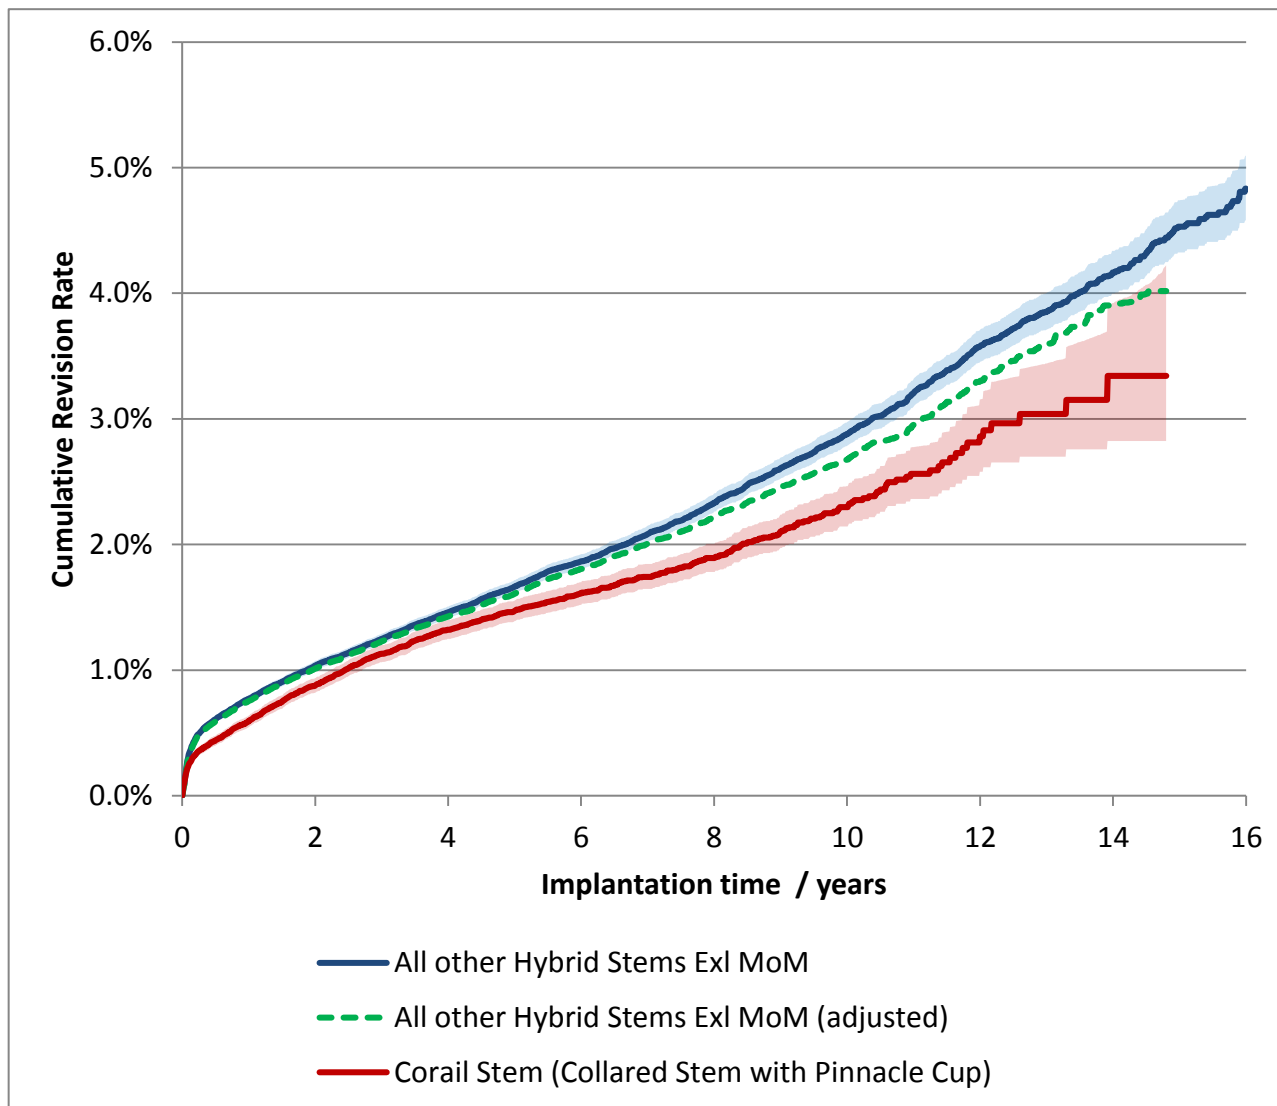


Cox Proportional Hazards model for revision risk ratio of Corail Stem (Collared Stem with Pinnacle Cup) / All other Hybrid Stems Exl MoM, with endpoint as any revision.

Adjustment	Hazard Ratio (95% CI)	p-value
Excluding MoM, Unadjusted.	0.77 (0.73 - 0.82)	<0.001
Excluding MoM. Adjusted for age, gender, year cohort and indications.	0.81 (0.77 - 0.86)	<0.001

**Revision and Survivorship**

**Cumulative Revision Rate**

Endpoint: Femoral Revision. Excluding Metal-on-Metal

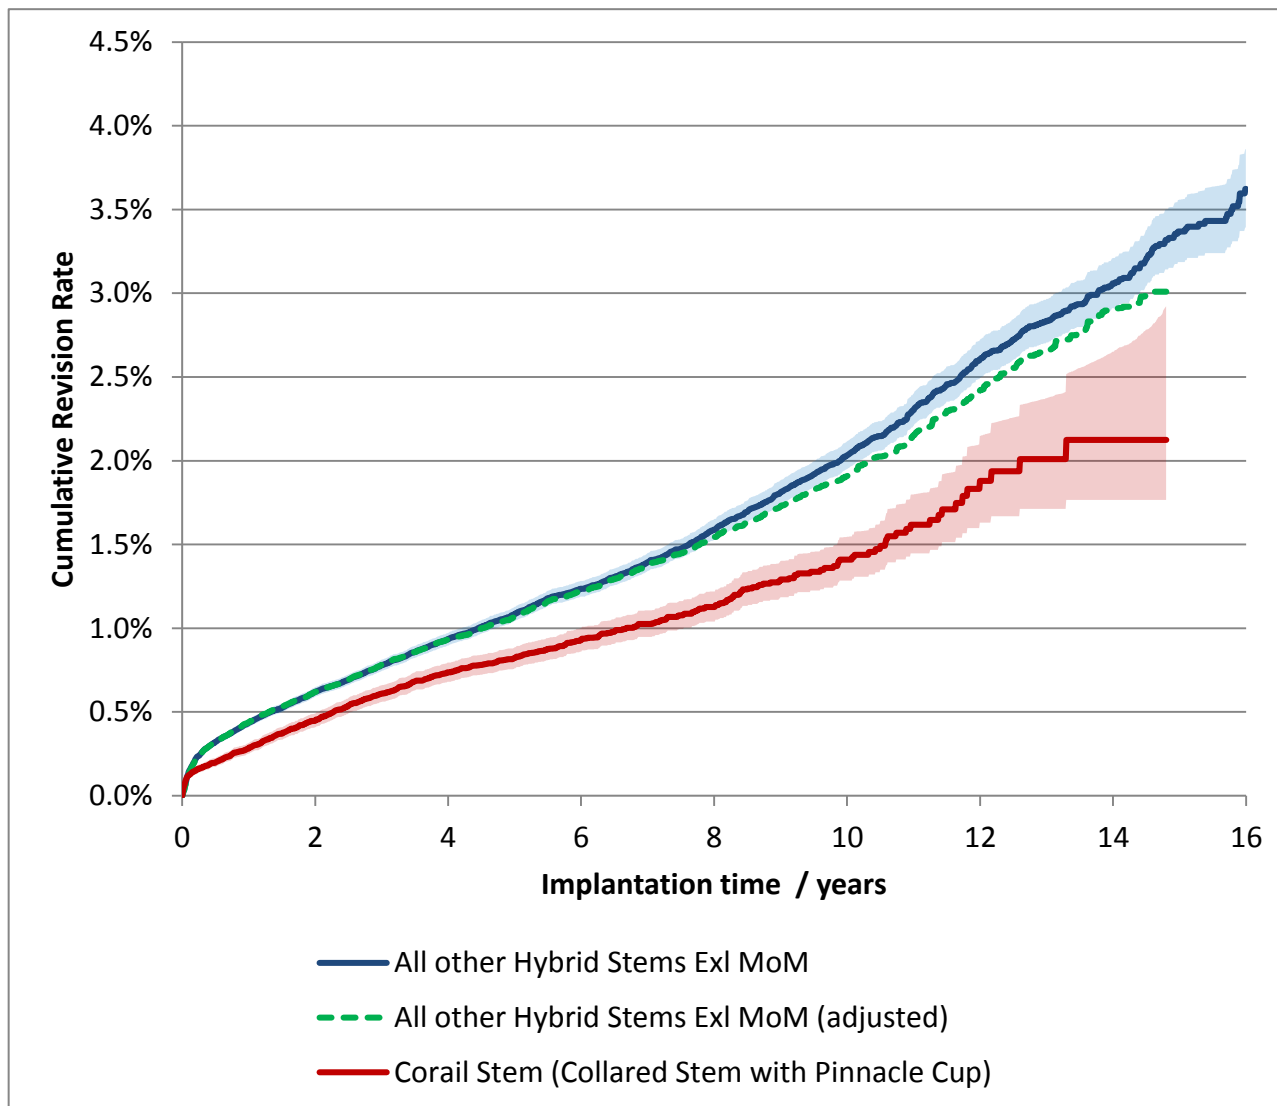

Cox Proportional Hazards model for revision risk ratio of Corail Stem (Collared Stem with Pinnacle Cup) / All other Hybrid Stems Exl MoM, with endpoint as any revision.

Adjustment	Hazard Ratio (95% CI)	p-value
Excluding MoM. Unadjusted.	0.67 (0.63 - 0.73)	<0.001
Excluding MoM. Adjusted for age, gender, year cohort and indications.	0.70 (0.65 - 0.76)	<0.001

Revision and Survivorship

Cumulative Revision Rate

Excluding Metal on Metal Bearings

Period /years	Endpoint: Any component revised				Endpoint: Femoral revision			
	At Risk	Corail Stem (Collared Stem with Pinnacle Cup)	All other Hybrid Stems Exl MoM	All THR	At Risk	Corail Stem (Collared Stem with Pinnacle Cup)	All other Hybrid Stems Exl MoM	All THR
0	102,823	-	-	-	102,823	-	-	-
1	95,425	0.6% (0.5% - 0.6%)	0.8% (0.7% - 0.8%)	0.8% (0.8% - 0.8%)	95,425	0.3% (0.3% - 0.3%)	0.4% (0.4% - 0.5%)	0.5% (0.5% - 0.5%)
2	81,826	0.9% (0.8% - 0.9%)	1.0% (1.0% - 1.1%)	1.1% (1.1% - 1.1%)	81,826	0.4% (0.4% - 0.5%)	0.6% (0.6% - 0.7%)	0.7% (0.7% - 0.7%)
3	68,159	1.1% (1.1% - 1.2%)	1.2% (1.2% - 1.3%)	1.3% (1.3% - 1.4%)	68,159	0.6% (0.6% - 0.7%)	0.8% (0.7% - 0.8%)	0.9% (0.8% - 0.9%)
4	55,603	1.3% (1.2% - 1.4%)	1.5% (1.4% - 1.5%)	1.6% (1.5% - 1.6%)	55,603	0.7% (0.7% - 0.8%)	0.9% (0.9% - 1.0%)	1.0% (1.0% - 1.0%)
5	43,732	1.5% (1.4% - 1.6%)	1.7% (1.6% - 1.7%)	1.8% (1.8% - 1.8%)	43,732	0.8% (0.8% - 0.9%)	1.1% (1.0% - 1.1%)	1.2% (1.1% - 1.2%)
6	33,706	1.6% (1.5% - 1.7%)	1.9% (1.8% - 1.9%)	2.0% (2.0% - 2.0%)	33,706	0.9% (0.9% - 1.0%)	1.2% (1.2% - 1.3%)	1.3% (1.3% - 1.3%)
7	24,920	1.7% (1.6% - 1.8%)	2.1% (2.0% - 2.1%)	2.3% (2.2% - 2.3%)	24,920	1.0% (0.9% - 1.1%)	1.4% (1.3% - 1.4%)	1.5% (1.4% - 1.5%)
8	17,767	1.9% (1.8% - 2.0%)	2.3% (2.3% - 2.4%)	2.5% (2.5% - 2.6%)	17,767	1.1% (1.0% - 1.2%)	1.6% (1.5% - 1.7%)	1.7% (1.6% - 1.7%)
9	11,906	2.1% (2.0% - 2.2%)	2.6% (2.5% - 2.7%)	2.8% (2.8% - 2.9%)	11,906	1.3% (1.2% - 1.4%)	1.8% (1.7% - 1.9%)	1.9% (1.8% - 1.9%)
10	7,259	2.3% (2.1% - 2.5%)	2.9% (2.8% - 3.0%)	3.1% (3.1% - 3.2%)	7,259	1.4% (1.3% - 1.5%)	2.0% (2.0% - 2.1%)	2.1% (2.0% - 2.1%)
11	3,965	2.6% (2.4% - 2.8%)	3.2% (3.1% - 3.3%)	3.5% (3.4% - 3.5%)	3,965	1.6% (1.4% - 1.8%)	2.3% (2.2% - 2.4%)	2.3% (2.3% - 2.4%)
12	2,016	2.9% (2.6% - 3.2%)	3.6% (3.5% - 3.7%)	3.9% (3.9% - 4.0%)	2,016	1.9% (1.6% - 2.1%)	2.6% (2.5% - 2.7%)	2.6% (2.6% - 2.7%)
13	1,050	3.0% (2.7% - 3.4%)	3.9% (3.7% - 4.0%)	4.3% (4.3% - 4.4%)	1,050	2.0% (1.7% - 2.4%)	2.8% (2.7% - 3.0%)	2.9% (2.8% - 3.0%)
14	474	3.3% (2.8% - 3.9%)	4.2% (4.0% - 4.3%)	4.7% (4.7% - 4.8%)	474	2.1% (1.8% - 2.7%)	3.1% (2.9% - 3.2%)	3.2% (3.1% - 3.2%)
15		( - )	4.5% (4.3% - 4.7%)	5.2% (5.1% - 5.3%)		( - )	3.4% (3.2% - 3.6%)	3.5% (3.4% - 3.6%)



Cumulative revision rate with 95% confidence intervals

Rate is only reported for times where more than 40 remain at risk

Patient Reported Outcomes

Comprising PROMs data up to and including: 31/12/2019

PROMs Analysis

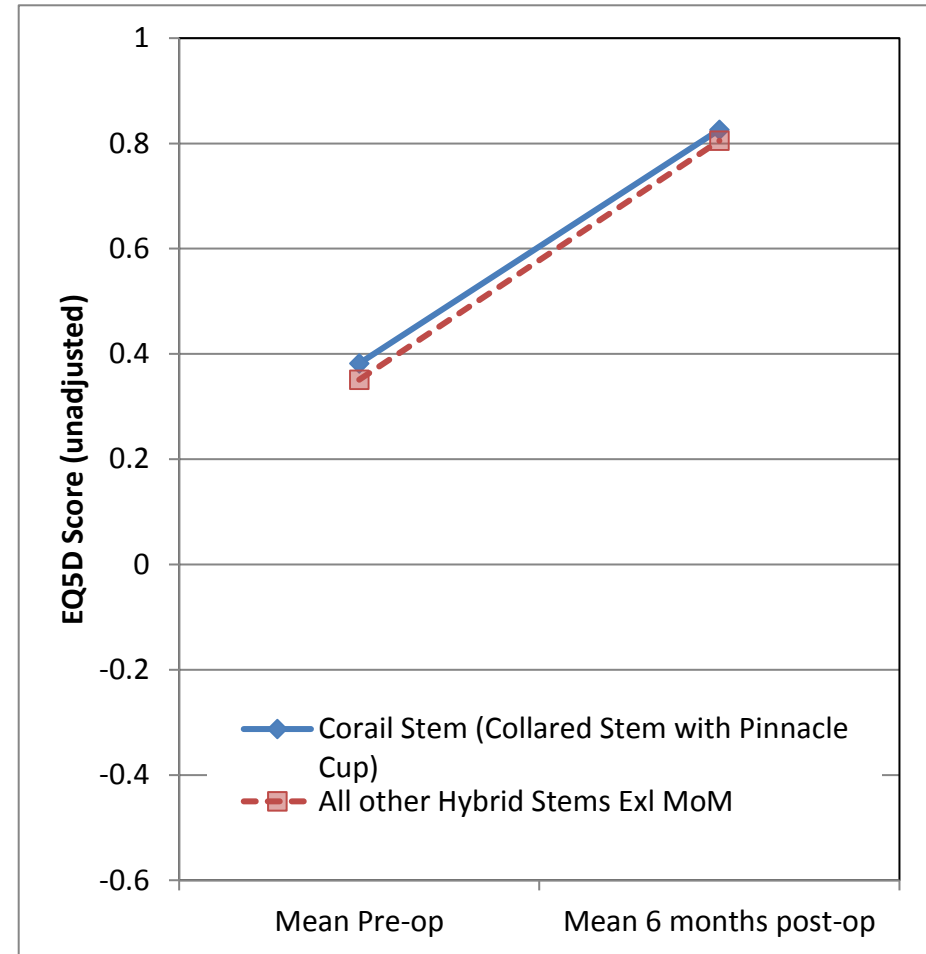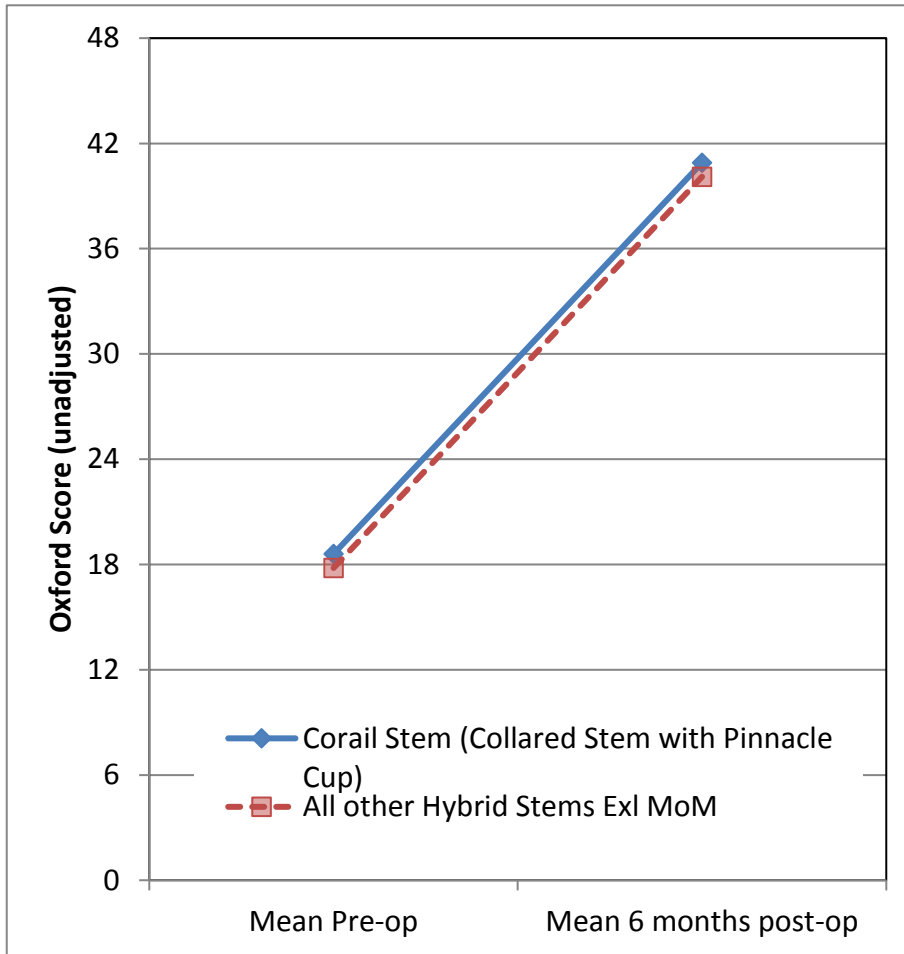



## Patient Reported Outcomes

## PROMs Analysis

Comprising PROMs data up to and including: 31/12/2019

Oxford Hip Score (0 - 48)	Corail Stem (Collared Stem with Pinnacle Cup)	All other Hybrid Stems Exl MoM	All THR in NJR
Paired Records	33,972	79,194	342,959
PreOp score	18.6 (18.5 - 18.7)	17.8 (17.8 - 17.9)	17.9 (17.9 - 18.0)
6 month score	40.9 (40.8 - 41.0)	40.1 (40.0 - 40.1)	39.5 (39.5 - 39.5)
6 month score (adjusted)	40.3 (40.3 - 40.4)	40.1 (40.0 - 40.1)	39.5 (39.5 - 39.5)
Health gain	22.3 (22.2 - 22.4)	22.2 (22.2 - 22.3)	21.6 (21.5 - 21.6)
Health gain (adjusted)	22.4 (22.3 - 22.5)	22.1 (22.1 - 22.2)	21.6 (21.5 - 21.6)
p value (adjusted health gain)	< 0.001		
Score Improved	97.8%	97.8%	97.3%

EQ-5D Index (-0.59 - 1.00)	Corail Stem (Collared Stem with Pinnacle Cup)	All other Hybrid Stems Exl MoM	All THR in NJR
Paired Records	31,382	72,992	315,677
PreOp score	0.382 (0.379 - 0.386)	0.351 (0.348 - 0.353)	0.353 (0.352 - 0.354)
6 month score	0.826 (0.824 - 0.829)	0.805 (0.804 - 0.807)	0.794 (0.794 - 0.795)
6 month score (adjusted)	0.813 (0.811 - 0.816)	0.805 (0.803 - 0.806)	0.794 (0.794 - 0.795)
Health gain	0.444 (0.440 - 0.448)	0.455 (0.452 - 0.457)	0.441 (0.440 - 0.442)
Health gain (adjusted)	0.460 (0.458 - 0.462)	0.452 (0.450 - 0.453)	0.441 (0.441 - 0.442)
p value (adjusted health gain)	< 0.001		
Score Improved	91.0%	90.7%	89.7%

EQ-VAS (0 - 100)	Corail Stem (Collared Stem with Pinnacle Cup)	All other Hybrid Stems Exl MoM	All THR in NJR
Paired Records	30,212	70,223	303,007
PreOp score	66.2 (66.0 - 66.5)	64.6 (64.5 - 64.8)	64.8 (64.7 - 64.9)
6 month score	79.0 (78.8 - 79.2)	77.6 (77.4 - 77.7)	77.0 (76.9 - 77.1)
6 month score (adjusted)	77.9 (77.7 - 78.0)	77.6 (77.4 - 77.7)	77.0 (76.9 - 77.0)
Health gain	12.8 (12.5 - 13.0)	13.0 (12.8 - 13.1)	12.2 (12.1 - 12.3)
Health gain (adjusted)	13.1 (12.9 - 13.2)	12.8 (12.7 - 12.9)	12.2 (12.1 - 12.3)
p value (adjusted health gain)	< 0.001		
Score Improved	67.8%	67.7%	66.4%

Adjusted scores correspond to the NHS Digital version 3 casemix-adjustment model. This includes patient variables from PROMs, HES, and IMD data.

Figures in parentheses represent the 95% confidence interval for the mean

Bespoke Report for:

Corail Stem (Collared Stem with Pinnacle Cup)

Responses are not case mix adjusted

**Patient Reported Outcomes**



## Patient Reported Outcomes

### Success

Response	Corail Stem (Collared Stem with Pinnacle Cup)	All other Hybrid Stems Exl MoM
Much better	31182	71420
A little better	2359	6014
About the same	608	1559
A little worse	315	897
Much worse	264	603

Answer to 6-months general health question:

"Overall, how are your problems now, compared to before your operation?"

### Satisfaction

Response	Corail Stem (Collared Stem with Pinnacle Cup)	All other Hybrid Stems Exl MoM
Excellent	16864	35974
Very Good	11380	27449
Good	4622	12058
Fair	1416	3830
Poor	424	1033

Answer to 6-months general health question:

"How would you describe the results of your operation?"

## Disclaimer

### Disclaimer

The National Joint Registry (NJR) produces this report through its contractor, Northgate Public Services (UK) Limited (NPS) using data collected, collated and provided by third parties. As a result, neither NJR or NPS takes any responsibility for the accuracy, currency, reliability and correctness of any data used or referred to in this report, and disclaims all warranties in relation to such data, in each case to the maximum extent permitted by legislation.

To the maximum extent permitted by law, neither the NJR or NPS shall have any liability (including but not limited to liability by reason of negligence) for any loss, damage, cost or expense incurred or arising by reason of any person using or relying on the data within this report and whether caused by reason of any error, omission or misrepresentation in the report or otherwise. This report is not to be taken as advice. Third parties using or relying on the data in this report do so at their own risk and will be responsible for making their own assessment and should verify all relevant representations, statements and information with their own professional advisers.

## Appendix A: Component List

Catalogue Number	Description	Number Implanted
3L92498	Corail Collared Stem K8A 115mm	3374
3L92499	Corail Collared Stem K9A 130mm	6147
3L92500	Corail Collared Stem K10A 140mm	12926
3L92501	Corail Collared Stem K11A 145mm	19438
3L92502	Corail Collared Stem K12A 150mm	15794
3L92503	Corail Collared Stem K13A 155mm	7962
3L92504	Corail Collared Stem K14A 160mm	4066
3L92505	Corail Collared Stem K15A 165mm	1756
3L92506	Corail Collared Stem K16A 170mm	701
3L92508	Corail Collared Stem K18A 180mm	137
3L92521	Corail Collared Stem K20A 190mm	10
3L93709	Corail Collared Lateralised Coxa Vara Stem KLA9 130mm	2469
3L93710	Corail Collared Lateralised Coxa Vara Stem KLA10 140mm	4019
3L93711	Corail Collared Lateralised Coxa Vara Stem KLA11 145mm	6284
3L93712	Corail Collared Lateralised Coxa Vara Stem KLA12 150mm	5347
3L93713	Corail Collared Lateralised Coxa Vara Stem KLA13 155mm	2679
3L93714	Corail Collared Lateralised Coxa Vara Stem KLA14 160mm	1491
3L93715	Corail Collared Lateralised Coxa Vara Stem KLA15 165mm	644
3L93716	Corail Collared Lateralised Coxa Vara Stem KLA16 170mm	265
3L93718	Corail Collared Lateralised Coxa Vara Stem Size 18	21
3L93720	Corail Collared Lateralised Coxa Vara Stem Size 20	1
L971109	Corail 135 High Offset KHO (Collar) Size 9	291
L971110	Corail 135 High Offset KHO (Collar) Size 10	673
L971111	Corail 135 High Offset KHO (Collar) Size 11	1571
L971112	Corail 135 High Offset KHO (Collar) Size 12	1754
L971113	Corail 135 High Offset KHO (Collar) Size 13	1139
L971114	Corail 135 High Offset KHO (Collar) Size 14	788
L971115	Corail 135 High Offset KHO (Collar) Size 15	404
L971116	Corail 135 High Offset KHO (Collar) Size 16	216
L971118	Corail 135 High Offset KHO (Collar) Size 18	33
L971120	Corail 135 High Offset KHO (Collar) Size 20	12
L971208	Corail 125 Standard Neck SN (Collar) Size 8	65
L971209	Corail 125 Standard Neck SN (Collar) Size 9	74
L971210	Corail 125 Standard Neck SN (Collar) Size 10	74
L971211	Corail 125 Standard Neck SN (Collar) Size 11	9
L971212	Corail 125 Standard Neck SN (Collar) Size 12	7
L971213	Corail 125 Standard Neck SN (Collar) Size 13	1
L971308	Corail 135 Short Neck SN (Collar) Size 8	55
L971309	Corail 135 Short Neck SN (Collar) Size 9	35
L971310	Corail 135 Short Neck SN (Collar) Size 10	72
L971311	Corail 135 Short Neck SN (Collar) Size 11	9
L971312	Corail 135 Short Neck SN (Collar) Size 12	7
L971313	Corail 135 Short Neck SN (Collar) Size 13	3

189708-210917 EMEA

